



Material provided:





2 Blood collector strips



1 blue top

buffer 1



buffer 2



Buffer



1 small tube







2 pipettes (1 drop \approx 40 μ L)


* For minor XM reverse the blood samples: Minor = Donor Plasma + Recipient RBCs and perform the same procedure

N°1: PREPARATION OF BLOOD SAMPLES •

(MAJOR = Donor RBCs + Recipient plasma)








Recipient

Centrifuge blood tube (5 min at 1000g) in order to collect plasma (1):




(1) or serum if using a dry tube

N°2: PREPARATION OF MAJOR XM











OR



















Incubate 10 minutes at room temperature

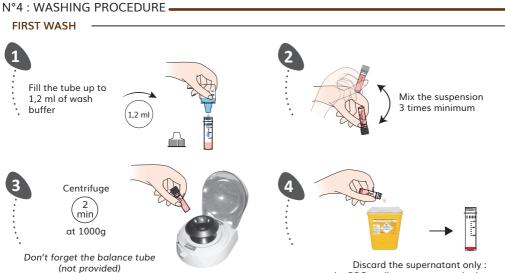



SECOND WASH

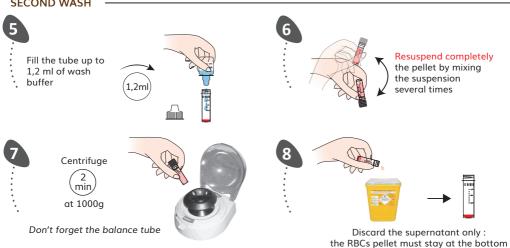

the RBCs pellet must stay at the bottom

THIRD WASH (PROCEDURE TO AVOID DILUTION BEFORE TESTING)

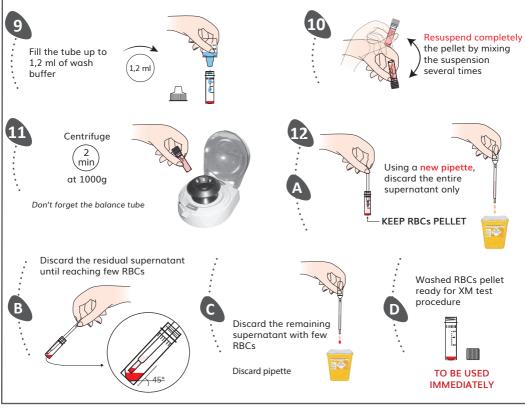

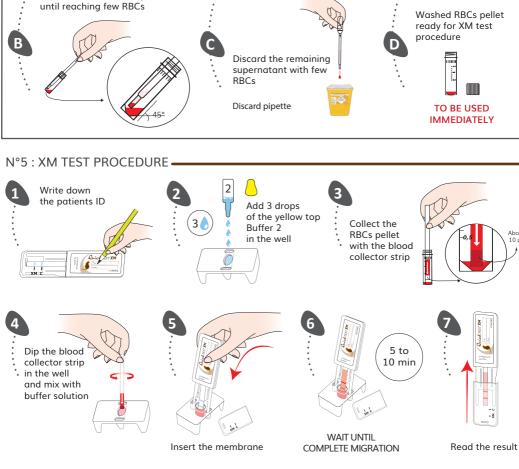

QuickTest XM

Result Interpretation



INCOMPATIBLE / DO NOT TRANSFUSE






Weak line = positive result



COMPATIBLE / SAFE TRANSFUSION





White line = negative result



In case of strong allo-antibodies in B cats plasma = positive result

C = Control Line / **XM** = Antiglobulin Test for detection of Feline CrossMatch

The XM test line will often be weaker than the control line.



In case of any other result, please take a picture and send us an email at : contact@alvedia.com www.alvedia.com

SCIENTIFIC ADVISES

It is MANDATORY to blood type the donor and the recipient before making a Feline XM Test.

Always transfuse COMPATIBLE blood.

Be careful, low titer and/or low affinity alloantibodies can be eluted during washing step procedures. This can affect the sensitivity of the XM test (e.g. low affinity/titer of anti-B in A blood group cat's plasma).

Usually, these alloantibodies cannot induce severe or mild hemolytic transfusion reaction.

Troubleshooting:
Please contact the
Scientific Service Laboratory
contact@alvedia.com
+33(0)478 380 239

